

Part of the  
**Aerobear®**  
Educational Series






*“Face mask seal is critical for efficient ventilation and aerosol delivery through holding chamber devices”\**



**Small**

**Medium**

**Large**

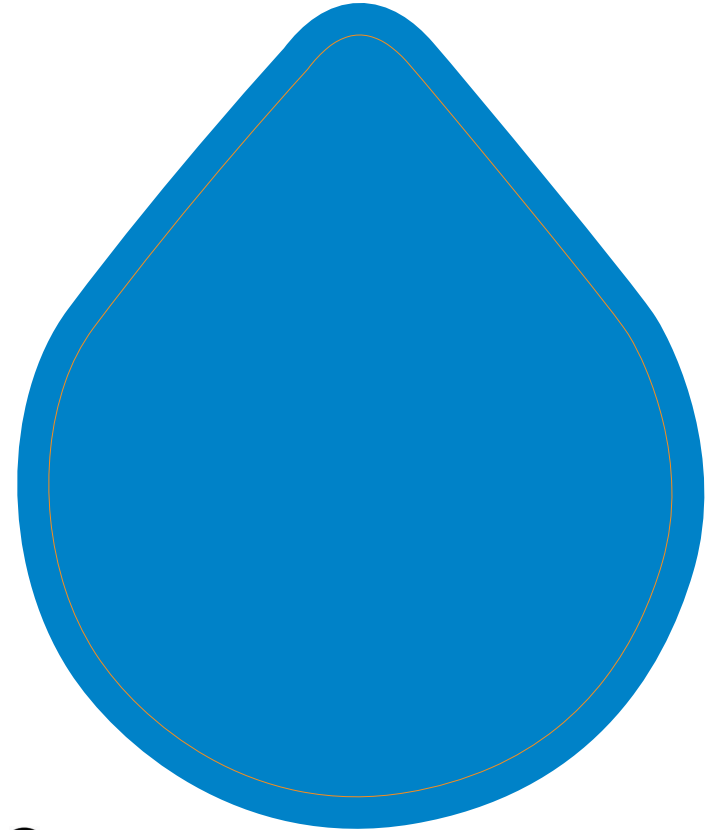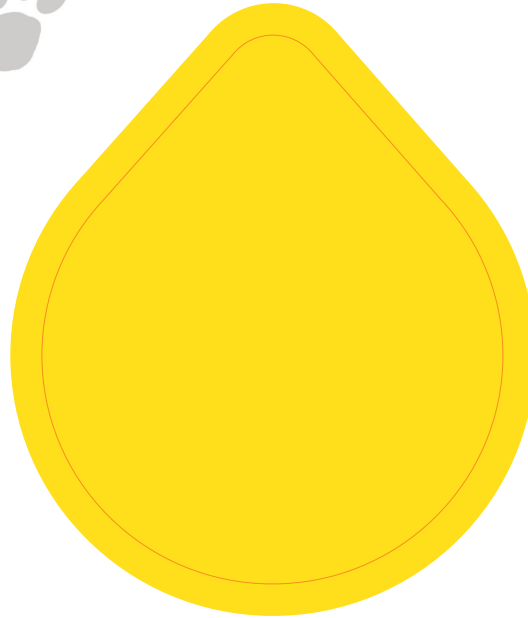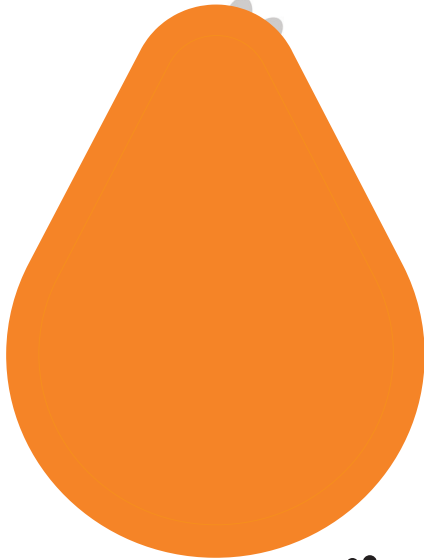


*AeroChamber*  
*Plus®* Z<sup>STAT</sup>™



**ComfortSeal® Mask Sizer**

©1999 Monaghan Medical Corporation. ® and ™ registered trademarks. PN 76317-02 11/07



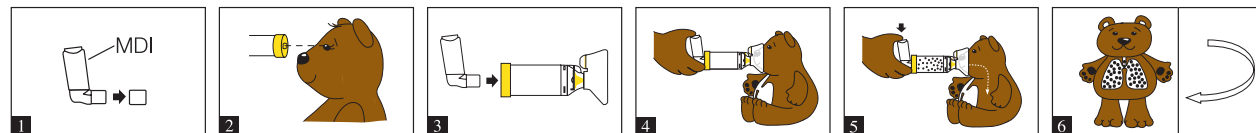


Monaghan Medical Corporation • 5 Latour Ave., Ste. 1600 • Plattsburgh, NY • 12901 1-800-833-9653

**AeroChamber  
MAX**

Part of the AerBear® Educational Series

**AeroChamber**  
*Plus*® Z<sup>STAT</sup>™

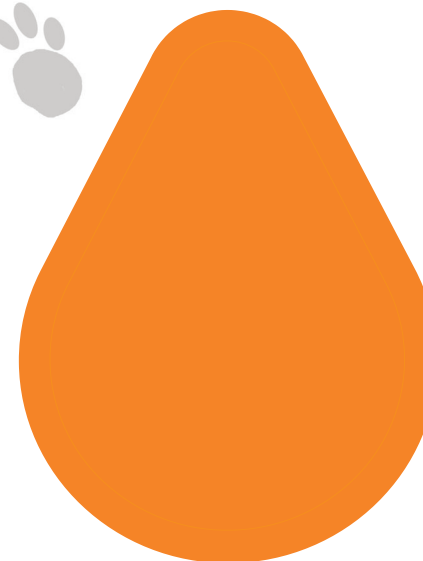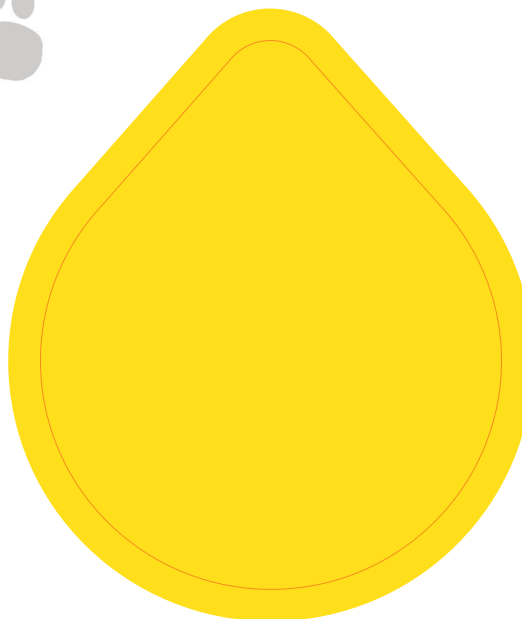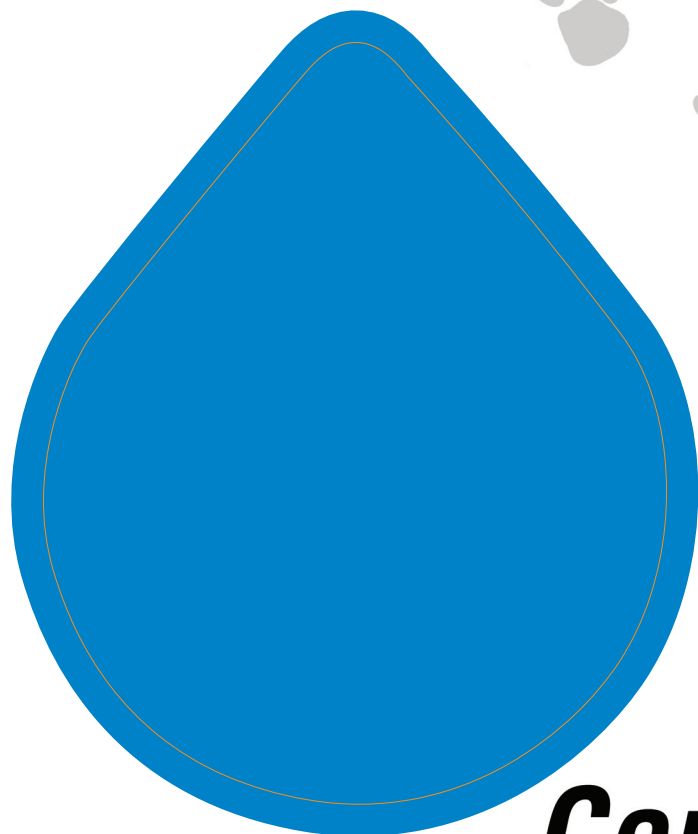

**monaghan**

***ComfortSeal*® Mask Sizer**

\* "Delivery of Aerosols to Children with MDI and Holding Chambers (MHC) is Critically Dependent on the Facemask Seal" Amirav et al, study presented at the ALA/ATS May 1999